



ANALIZA BIAŁEK



100006697

## Laboratory of Analysis

**Client:** Camo Chem  
**Order number:** 100006697  
**Name:** S23  
**Number of samples:** 1 vial

**Batch number:** -----  
**Recive date:** 2025-01-07  
**Start date:** 2025-01-08  
**End date:** 2025-01-09

## Sample identification

Substance	Method of taking a sample	Form
S23	Sample provided by customer	White powder in glass vial


## Results

Substance	Sample name	Content	Purity
S23	S23	-----	99%

## Research comment

The test sample was applied in the amount of 2  $\mu$ l to the BioBasic 8 Thermo Scientific column. During the analysis with the method a linear gradient in the solutions of H<sub>2</sub>O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its purity, when compared to the reference chromatogram, is 99%. The measurement error is + - 1%. The actual state of the sample sent before the test is presented on the photo below

## Photo of the test sample

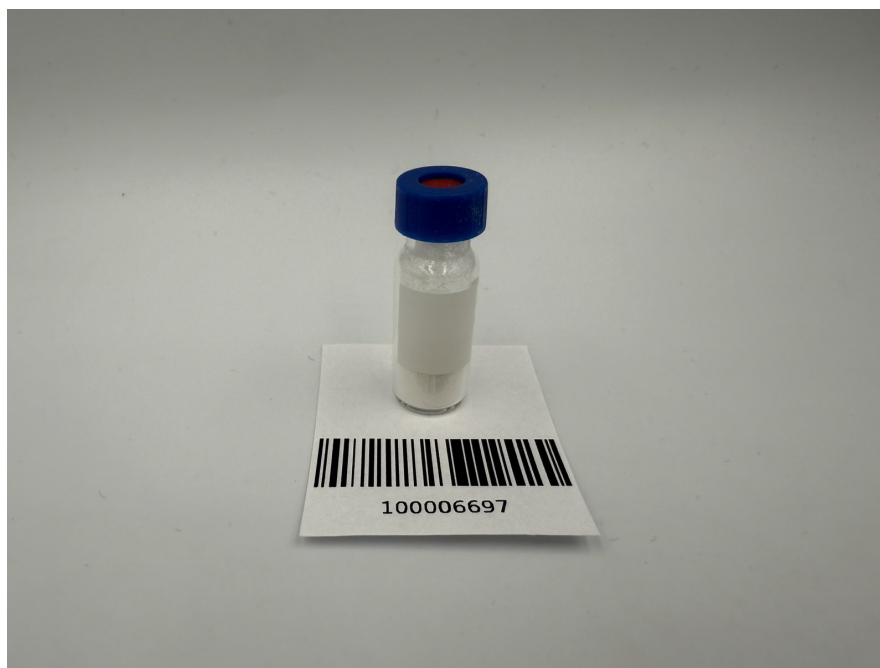

**Password**

2V9S8F7H


**Analiza Białek sp. z o.o.**  
**KRS:** 0000966168  
**NIP:** 8992922970  
**REGON:** 521751875

**Headquarters and Laboratory:**  
ul. Duńska 9, 54-427 Wrocław  
Budynek DELTA

**Lab technician:**  
Analysis and research specialist  
mgr Arkadiusz Zajęc



## Chromatogram

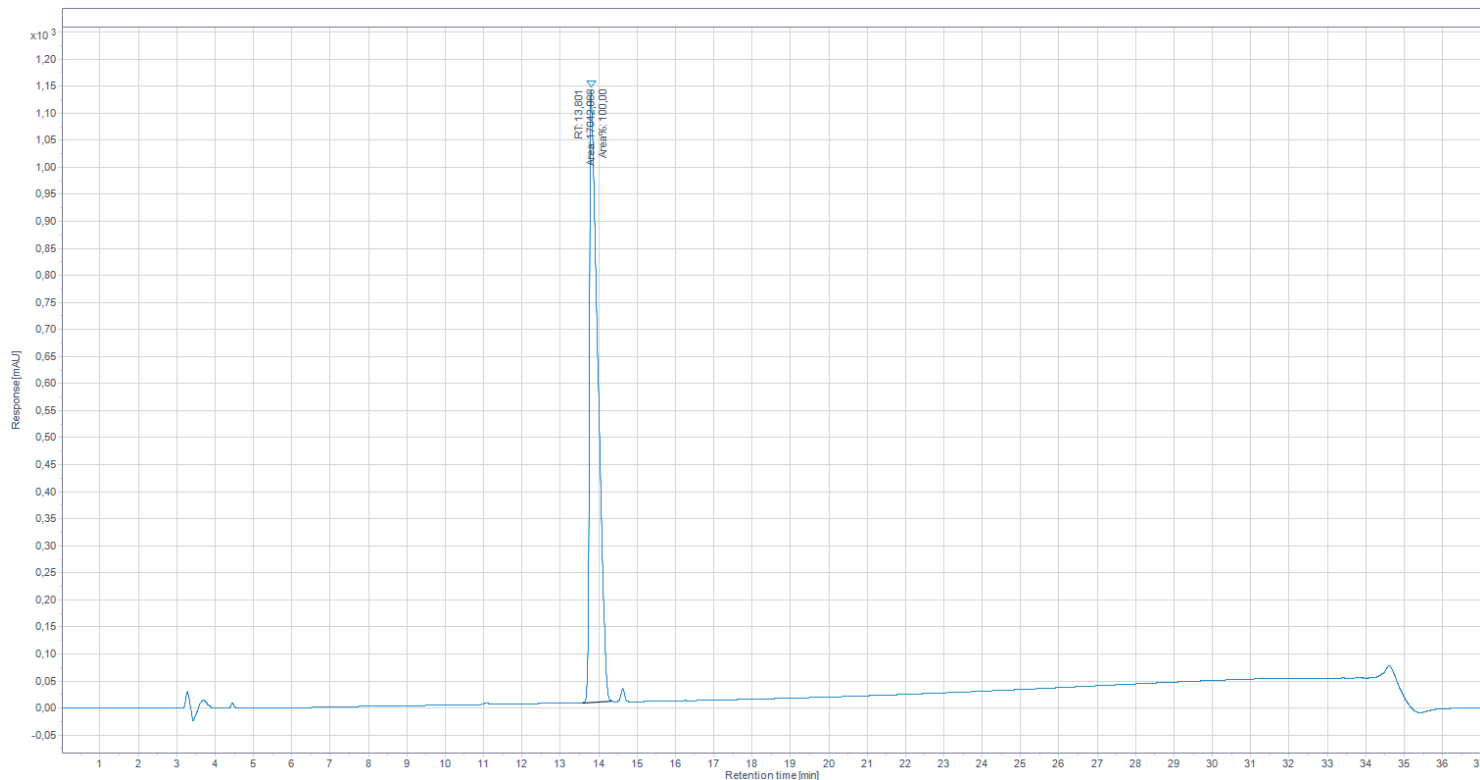

## Metoda

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

## Password

2V9S8F7H